






**Persona™ Fixed
Resection Tower
42-5099-006-00**

Cleaning Instructions

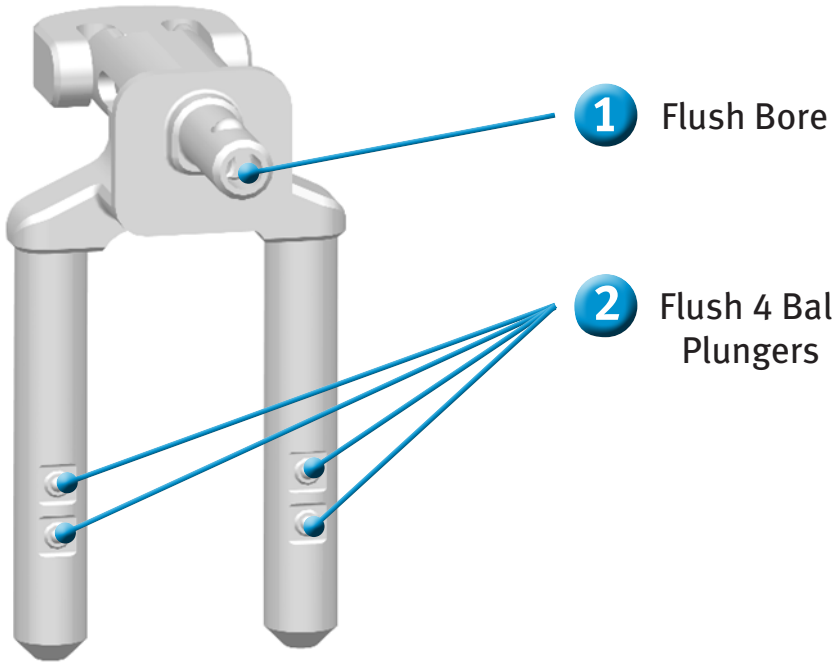

3 Flush Spring Cavity
(top and bottom)

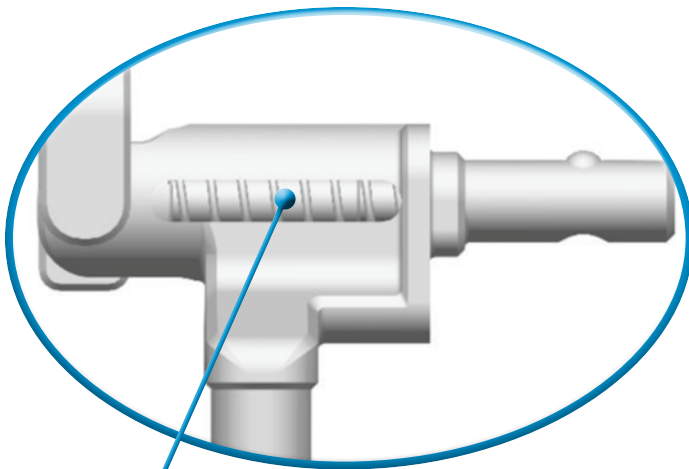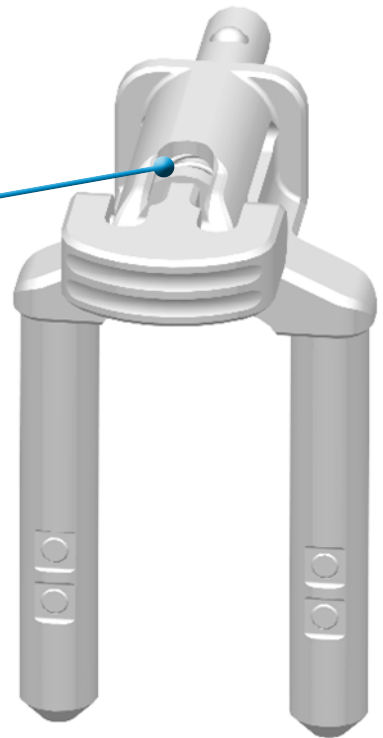

4 Flush Spring Cavity
(both sides)

97-5026-008-00 MC0000099147/00 Printed in USA ©2013 Zimmer, Inc.