




EM Distal Telescoping Tube 00-5901-071-00

Cleaning Instructions

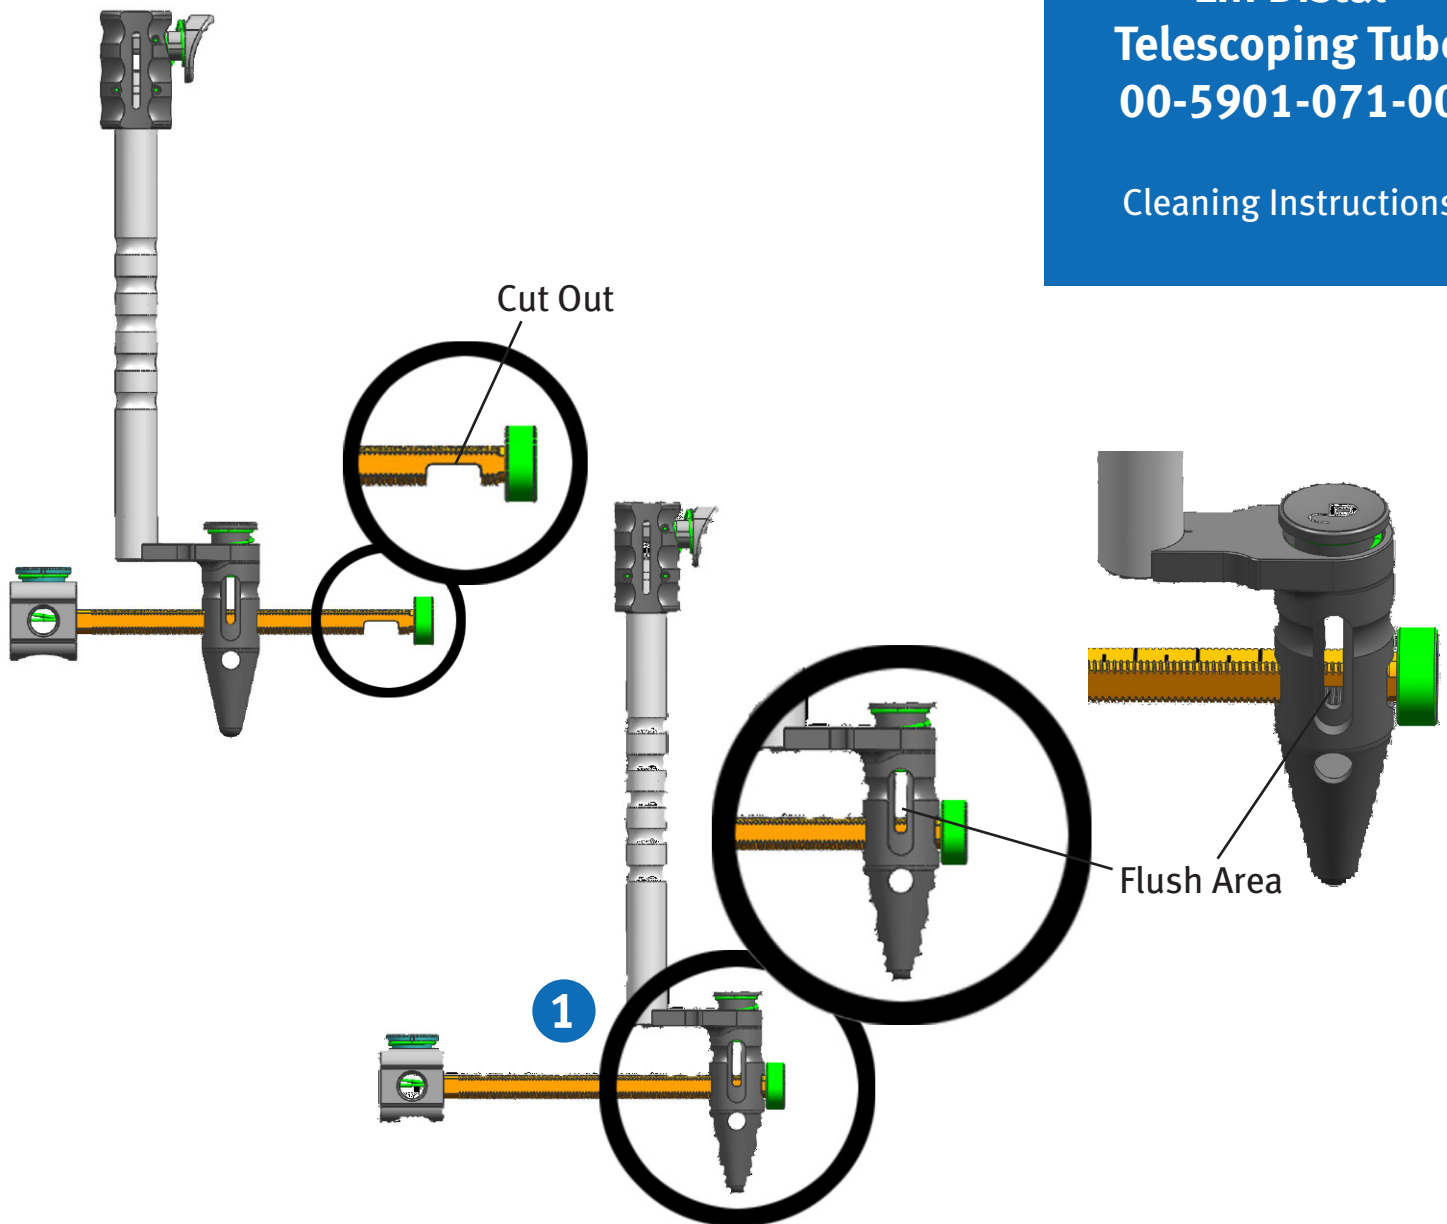

Move assembly to position **1** to access flushable area cut out.
Flush area shown.



+H124970000403001/\$100610F10K

97-0000-403-00 1003-K21 Printed in USA ©2010 Zimmer, Inc.

