


IMPORTANT: Remove drill stop from drill (42-5399-018-10) before cleaning and sterilization



**Persona™
Cemented Tibial Drill
Stop Collar, 15.7mm
42-5399-019-00**

Cleaning Instructions

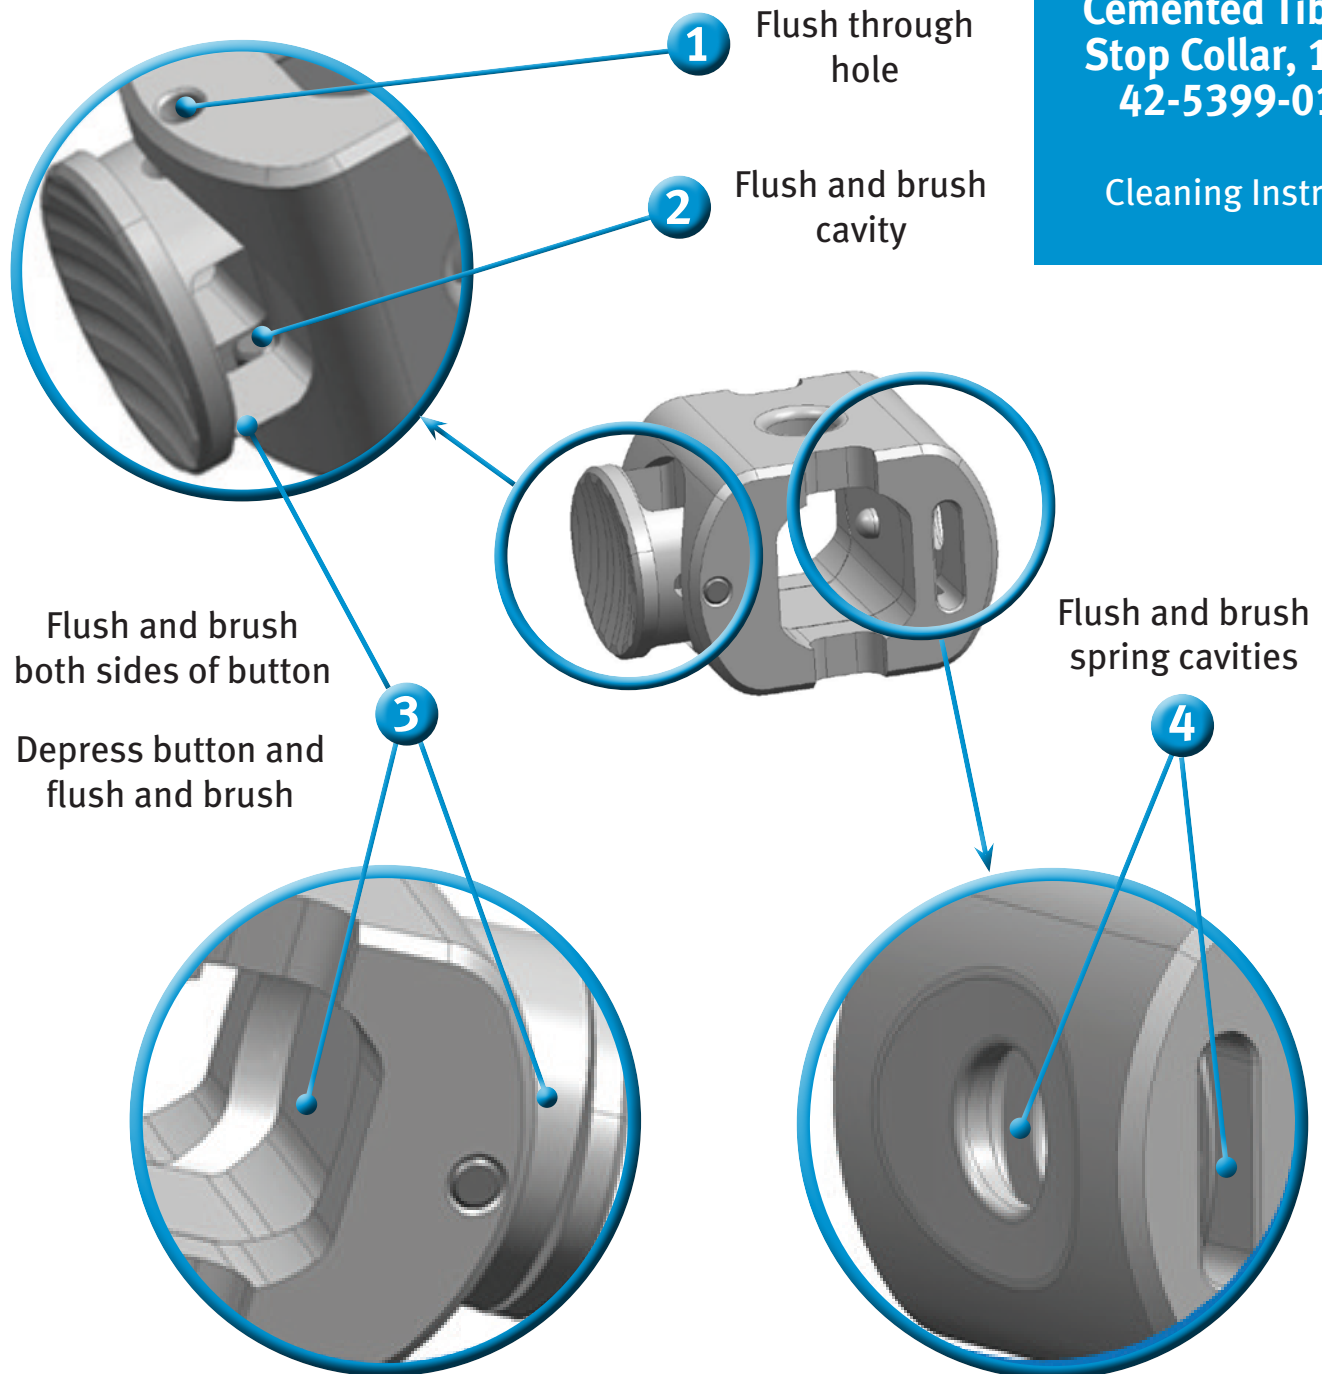

97-5026-069-00 Printed in USA ©2012 Zimmer, Inc.